



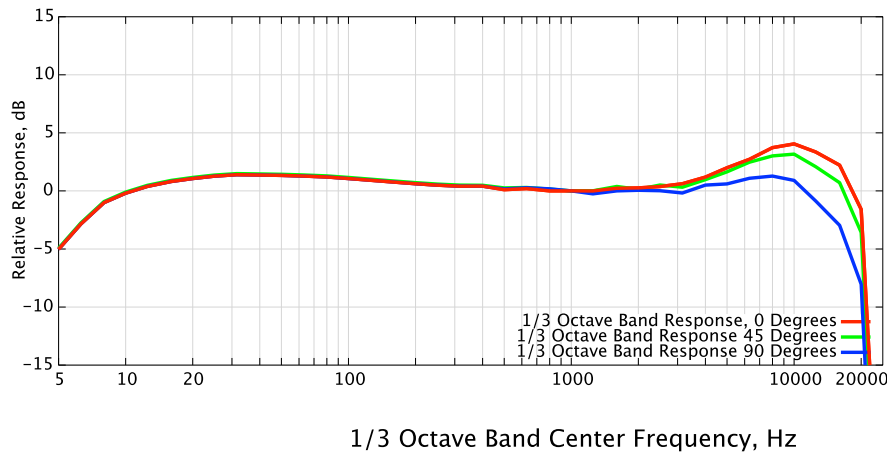

## Microphone Frequency Response Measurement Report

**Microphone Manufacturer:** miniDSP      **Model Number:** UMIK-1  
**Serial Number:** 700-2843      **Phantom Power:** USB  
  
**Measurement Date:** January 28, 2014      **Temperature:** 63°F/17°C  
**Engineer:** G. Holey      **Humidity:** 23%

1/3 OB Results	
Freq.	Resp. (dB)
5	-5.03
6.3	-2.84
8	-1.01
10	-0.20
12.5	0.39
16	0.81
20	1.06
25	1.27
31.5	1.40
40	1.37
50	1.34
63	1.28
80	1.20
100	1.06
125	0.92
160	0.76
200	0.62
250	0.50
315	0.41
400	0.41
500	0.10
630	0.20
800	0.01
1000	0.00
1250	-0.00
1600	0.23
2000	0.26
2500	0.37
3150	0.62
4000	1.19
5000	2.00
6300	2.73
8000	3.72
10000	4.05
12500	3.36
16000	2.22
20000	-1.59
25000	-35.74

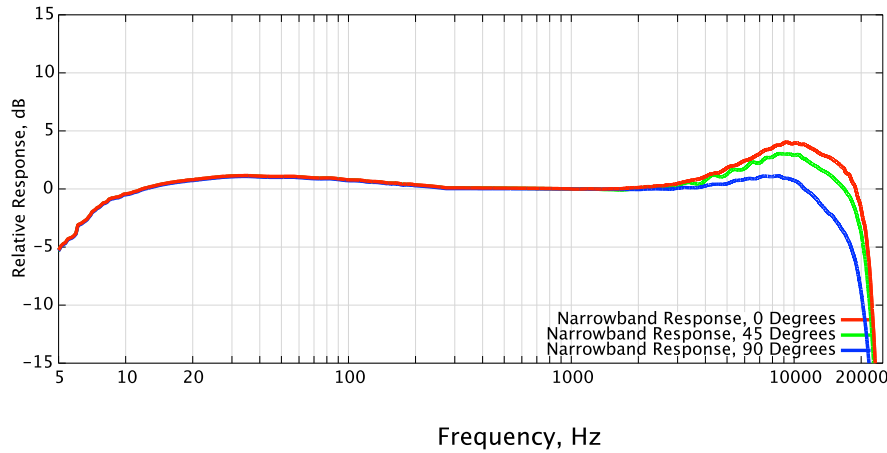

This frequency response measurement is not a NIST-traceable calibration.

### Reference Microphone

