


Sample Name: Mystery blend

```

=====
Acq. Operator   : SYSTEM                      Seq. Line :    2
Acq. Instrument : 6890N                      Location  : 102 (F)
Injection Date  : 2/23/2018 4:17:42 PM      Inj       :    1
                                                Inj Volume: 1 µl
Sequence File   : C:\Chem32\1\DATA\2018-02-23CY-5L2561\CY-5L2561.S
Method          : C:\Chem32\1\DATA\2018-02-23CY-5L2561\CY-5L2651 TEST.M (Sequence
                  Method)
Last changed    : 2/23/2018 4:14:54 PM by SYSTEM
=====

```

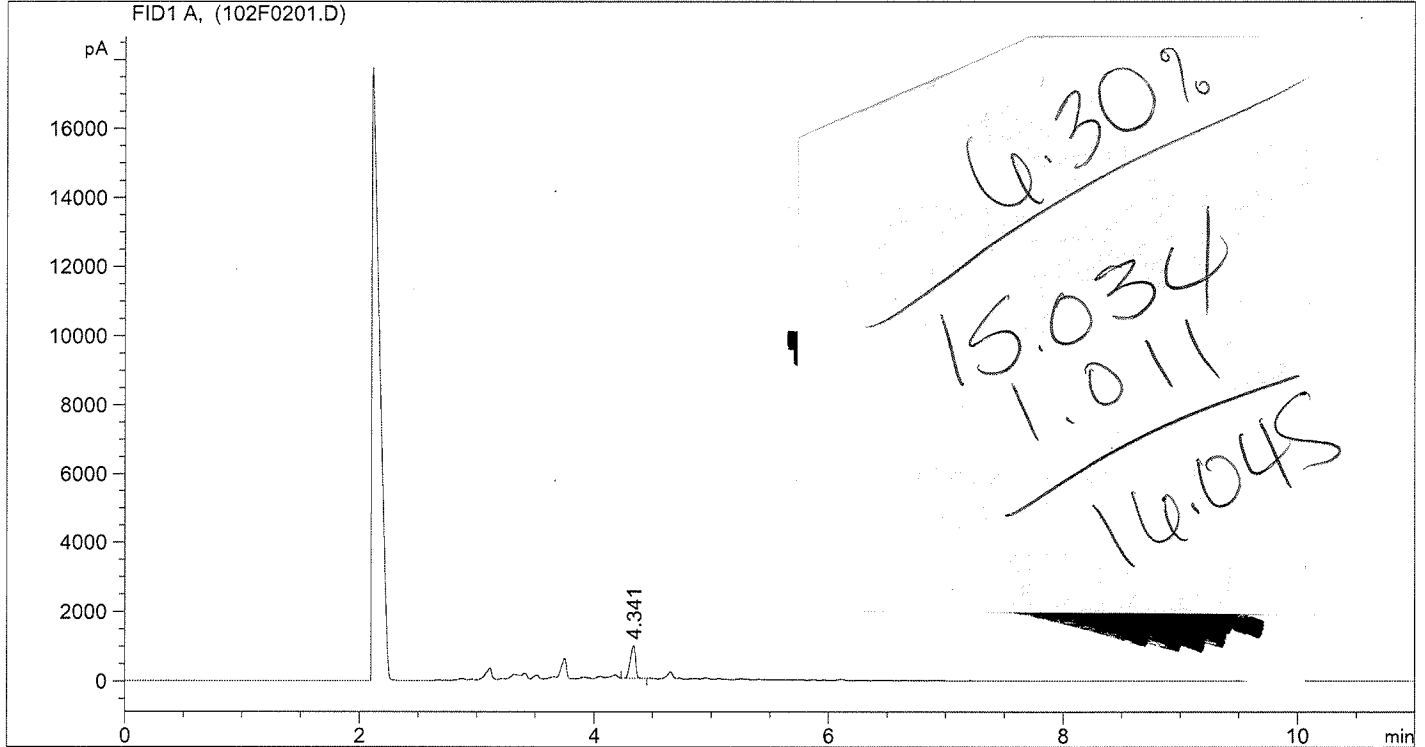

```

=====
External Standard Report (Sample Amount is 0!)
=====

```

```

Sorted By           : Signal
Calib. Data Modified : Friday, February 23, 2018 4:14:54 PM
Multiplier          : 1.0000
Dilution            : 1.0000
Use Multiplier & Dilution Factor with ISTDs

```

Signal 1: FID1 A,

RetTime [min]	Type	Area [pA*s]	Amt/Area	Amount [ng/ul]	Grp	Name
4.341	VBA+	2929.88281	2.13080e-3	6.24300		Hex-Ether
Totals :				6.24300		

\*\*\* End of Report \*\*\*