

CH1

0.000s

Trig

Acquire

Normal

Average

Peak Detect


Sample Rate  
250kS/s



1V

10ns

CH1 EDGE 1.00  
49.9341Hz

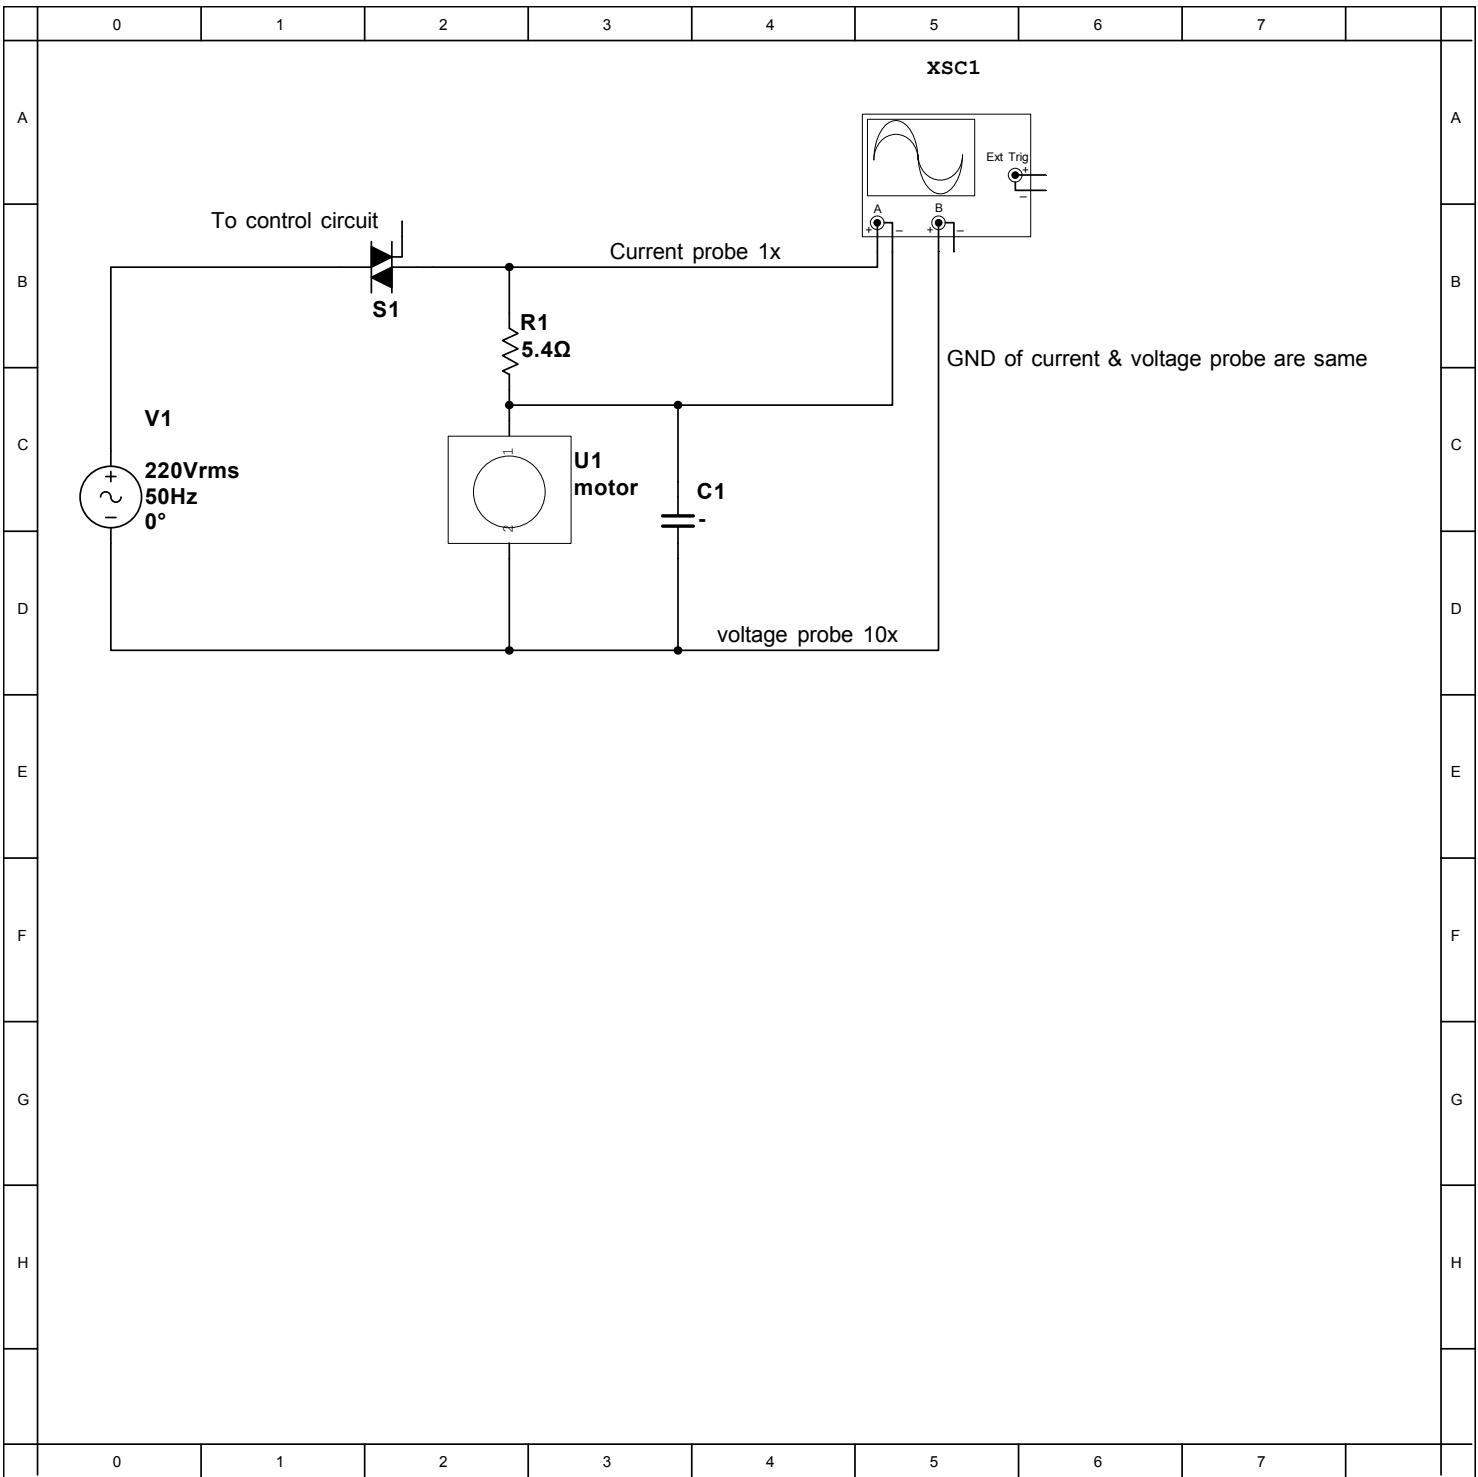




WINSTEK

▼ 0.000s

Trigger

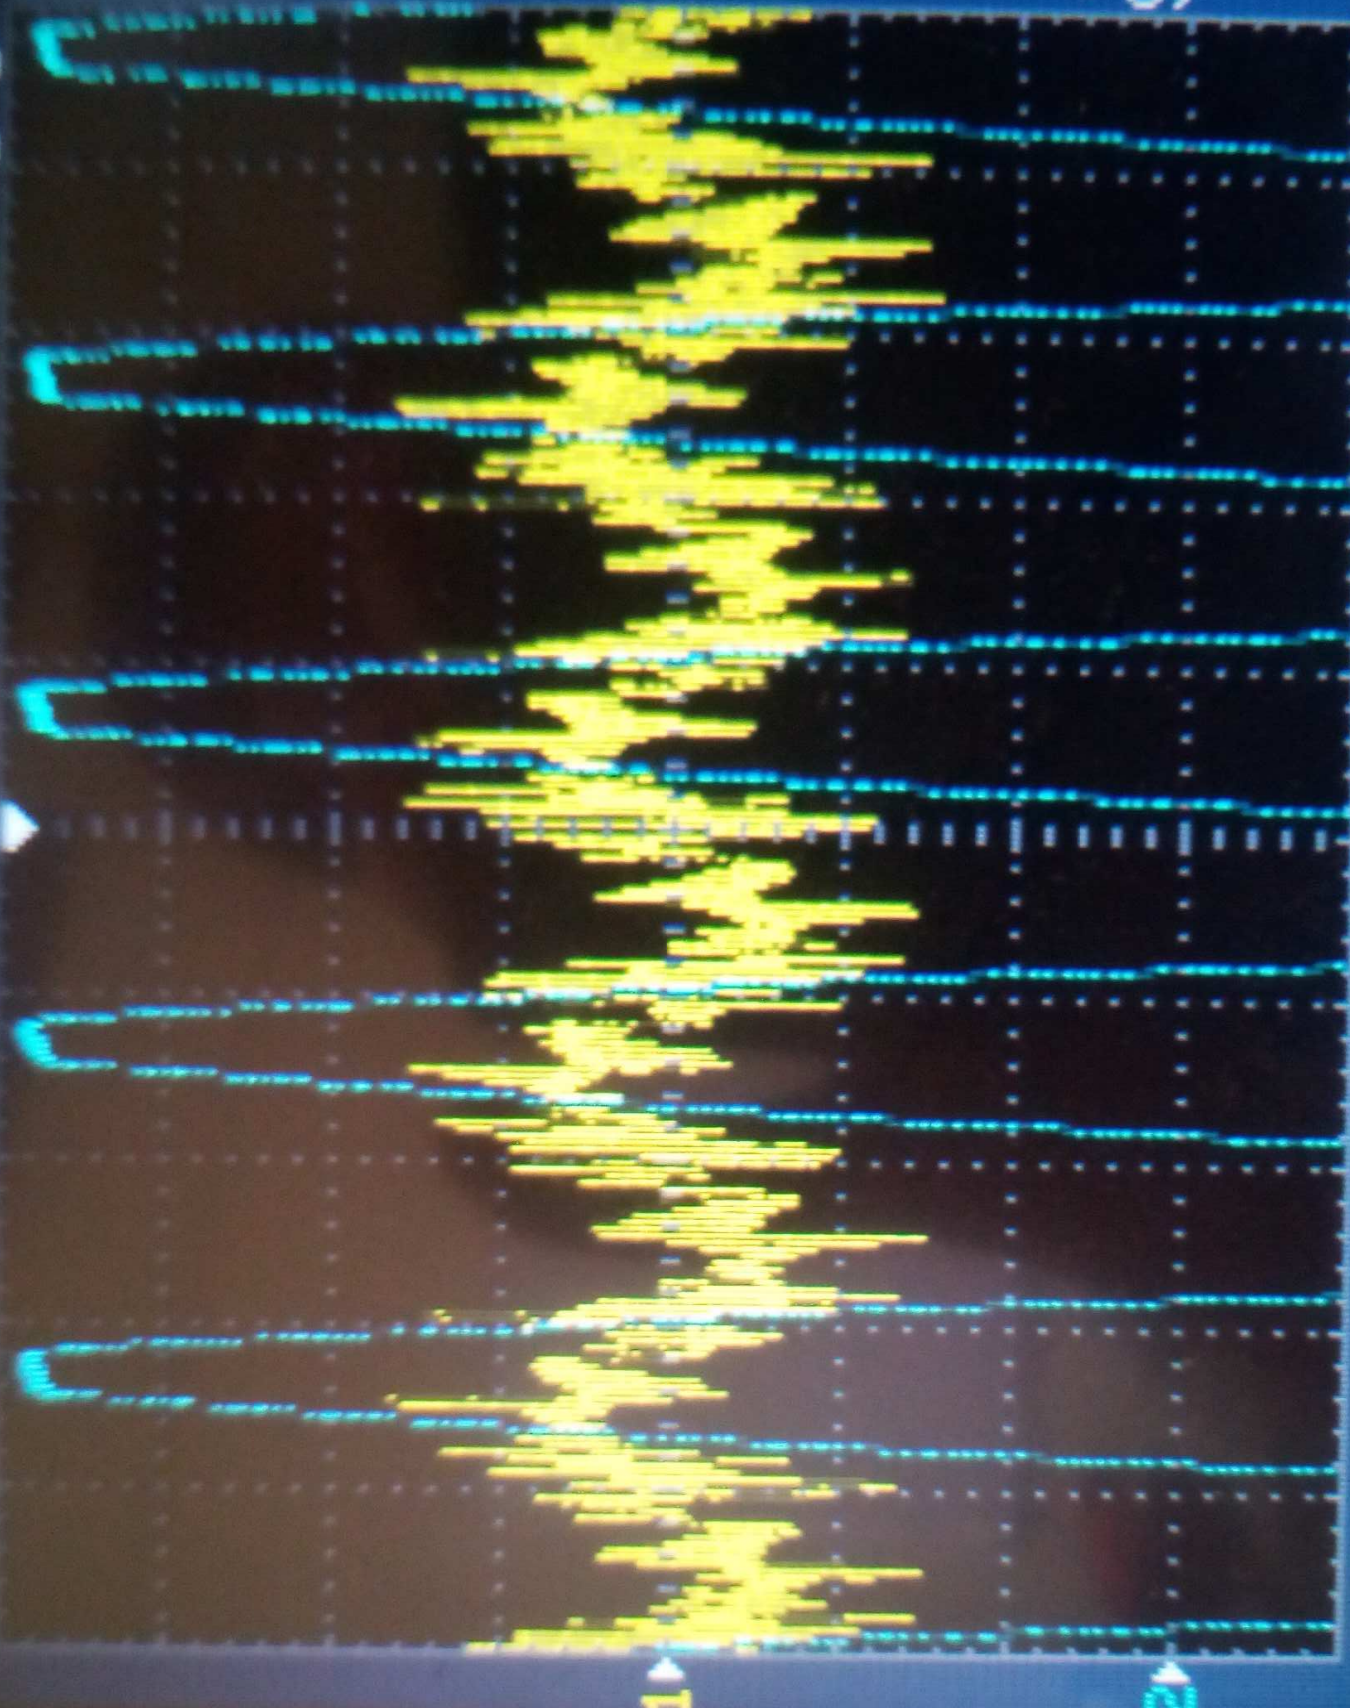

1V

10ms

CH1

San



MPER225V  
4500-5  
DS-SS



